USA E8 Combination Centrifuge

The E8 Combination Centrifuge is specifically designed to spin 75mm microhematocrit tubes and 1-15ml microtubes and test tubes. Its short height makes it easy to fit under any cabinet, and an auto-calibrating speed function gives precise results. In addition, the E8's quiet run cycles create a more peaceful laboratory environment.

To run microhematocrit tubes, simply insert your 75mm capillary tubes into the carrier, place carriers in opposing tubes sleeves for a balanced load, and spin at 3,500 rpm for 6 minutes for clear separation.



Accurate speeds for specific g-forces
Proper separations without cell damage
Quiet, vibration-free operation
Auto-brake stops the rotor in less than 30 seconds
Spins 8, 75mm capillary tubes
Designed, Engineered, and Assembled
Proudly in America



Angled rotor, 8-tube capacity
Holds 1ml to 15ml size tubes and
75mm capillary tubes
12 volt DC maintenance-free motor
Clear view port in lid for using tachometer
Suction-cupped feet prevent slipping
110/220v auto-switching power adapter
(CE, UL, cUL approved)
Lid safety shut-off switch
Maximum RCF=1,534g

WEIGHT AND DIMS

Height: 9.5" (241mm) Length: 11" (279mm) Width: 11" (279mm) Weight: 9.5 lbs (4.3kg)

INCLUDES

Eight-place rotor
Eight 5ml-15ml blue tube sleeves
Eight 3ml-4ml black tube sleeve inserts
Six green tube inserts to spin 1ml-2ml
Two 4-place Crit Carrier inserts
(75mm capillary tubes)
EZ Reader Card





USA E8 Combination Centrifuge

Model #	Description
E8C-U8AD-CRT3	USA E8 Digital-Speed, Angled 8-Place Centrifuge with Crit Carriers
E8C-U8AV-CR03	USA E8 Variable-Speed, Angled 8-Place Centrifuge with Crit Carriers
E8C-U8AF-CR03	USA E8 Fixed-Speed, Angled 8-Place Centrifuge with Crit Carriers

E8 FIXED SPEED

3,500rpm fixed speed - for blood only Auto-off 30-minute timer with bell

E8 VARIABLE SPEED

3,500 rpm with variable speed control knobs (blood, urines, microhematocrits, etc.)
Auto-off 30-minute timer with bell

E8 DIGITAL

3,500 rpm digital speed and time (blood, urines, microhematocrits, etc.) Touch pad, programmable:

Speed: 500-3,500rpm Time: 1-99mins

Stores last four programmed speeds & times


Service Indicator Light




P 770.270.1394 F 770.270.2389

865 Marathon Parkway Lawrenceville GA 30046

3 EASY STEPS TO ACHIEVE ACCURATE PCV RESULTS:








Insert the carrier in the blue tube sleeves.



Spin at 3,500 rpm for 6 (+/-1) minutes.

EXPLANATION OF MICROHEMATOCRITS IN AN ANGLED CENTRIFUGE:

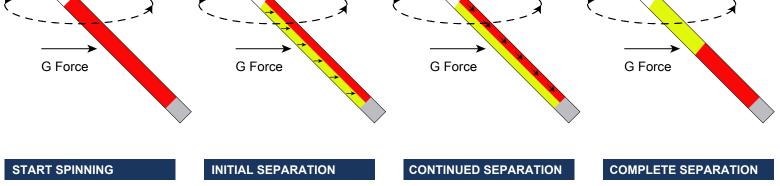

Red cells move outward.
Plasma moves inward.

Red cells pass plasma easily.

No trapped plasma. Accurate PCV results.

In a traditional microhematocrit centrifuge with a flat rotor, the red cells and the plasma must pass through each other horizontally in the narrow tube. In this case, very high speed and g-force is needed to reduce trapped plasma. When using LW Scientific Crit Carriers in an angled rotor, the red cells initially move to the outer tube wall while the plasma initially moves to the inner tube wall. Then, they pass each other easily as the red cells travel down to the bottom of the tube and the plasma travels to the top. With more efficient separation and ZERO trapped plasma, the PCV value will be accurate.

The E8 Combination Centrifuge is a FDA registered, Class II medical device.

Comparable results to the HemataStat II angled PCV centrifuge sold to the human market. The HemataStat II produces PCV results at 2,000 g-force in 1 minute.